


**LEVEL**  
23.10.2009  
17:46:07

Output: Analog  
Imp: 600Ohm  
Sine  
-0.00dBV 250.0 Hz

Input: Analog  
Imp: 100kOhm

Filter:  
Off

A: 0.45dBV 249.9 Hz

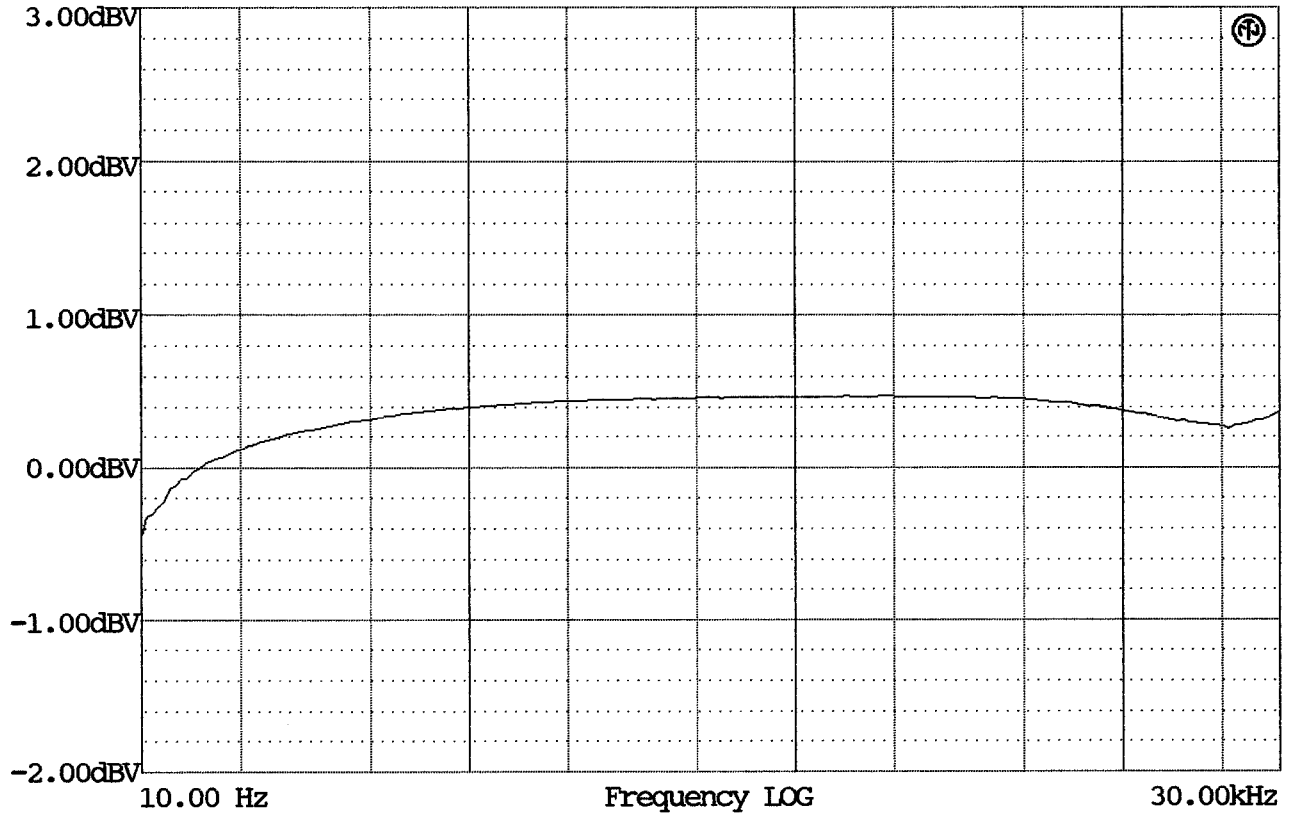


**THD+N**  
23.10.2009  
17:52:28

Output: Analog  
Imp: 600Ohm  
Sine  
-0.00dBV 250.0 Hz

Input: Analog  
Imp: 100kOhm

Filter:  
Off

A: 0.45dBV 249.9 Hz

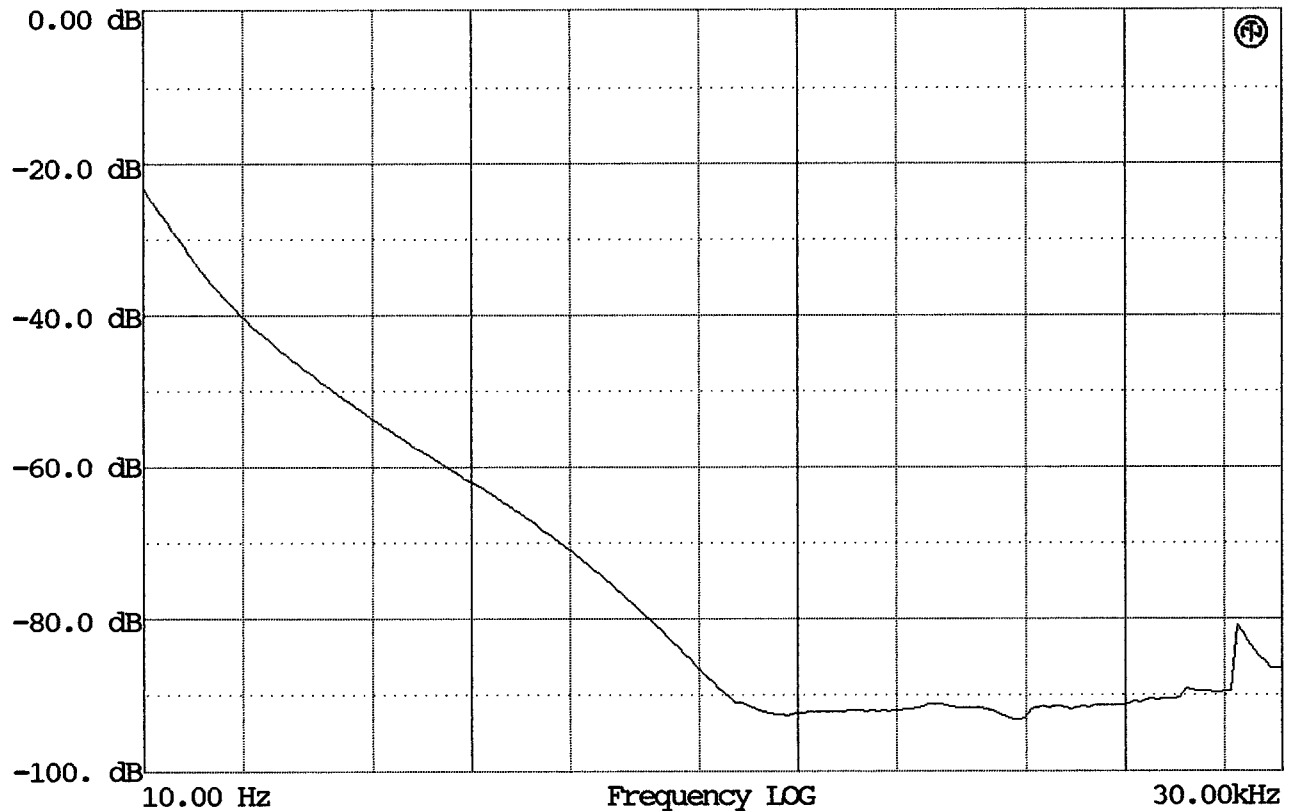

*DI 70x VES 02*


THD+N  
23.10.2009  
17:58:23

Output: Analog  
Imp: 600Ohm  
Sine  
10.0dBV 250.0 Hz

Input: Analog  
Imp:100kOhm

Filter:  
Off

A: 10.4dBV 249.9 Hz

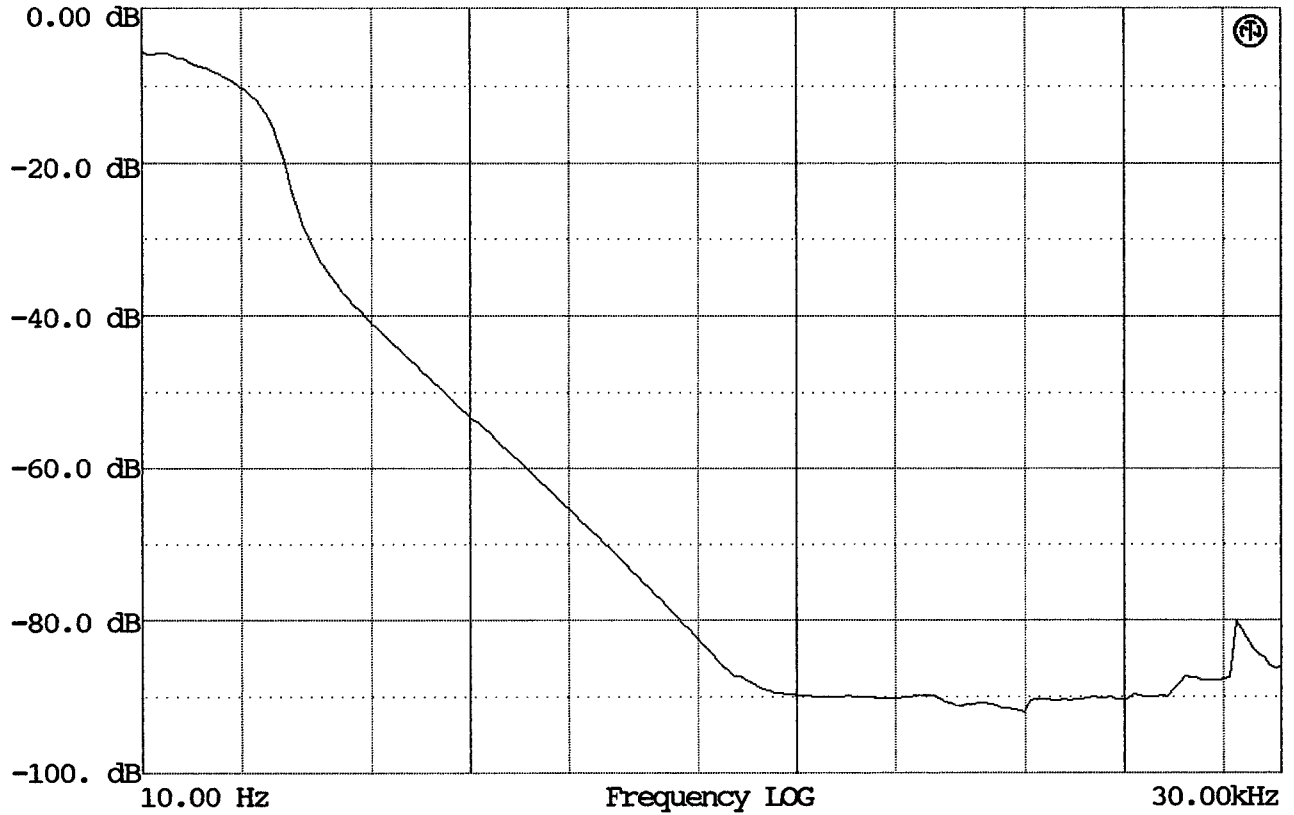


THD+N  
23.10.2009  
18:04:16

Output: Analog  
Imp: 600Ohm  
Sine  
-10.0dBV 250.0 Hz

Input: Analog  
Imp:100kOhm

Filter:  
Off

A: -9.55dBV 249.9 Hz

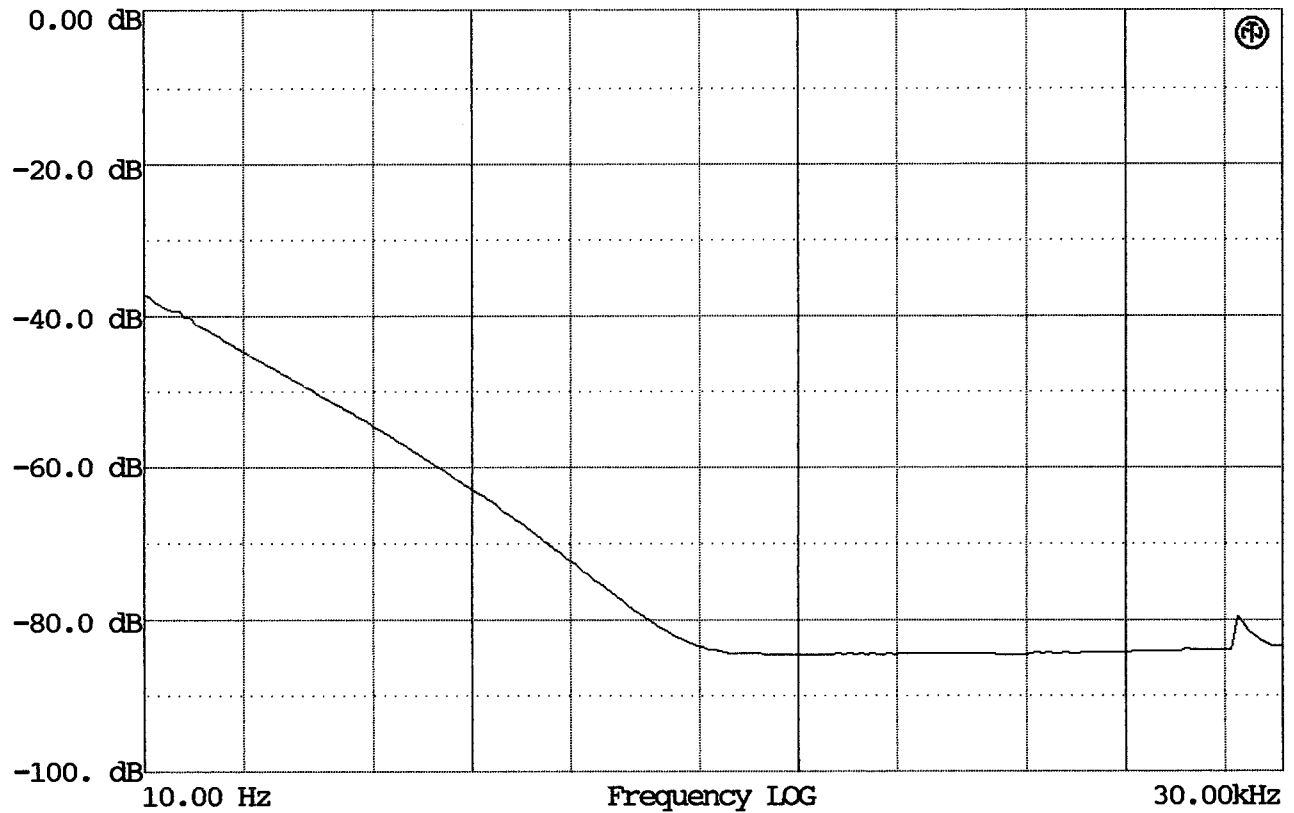

SI 70x U20CZ